
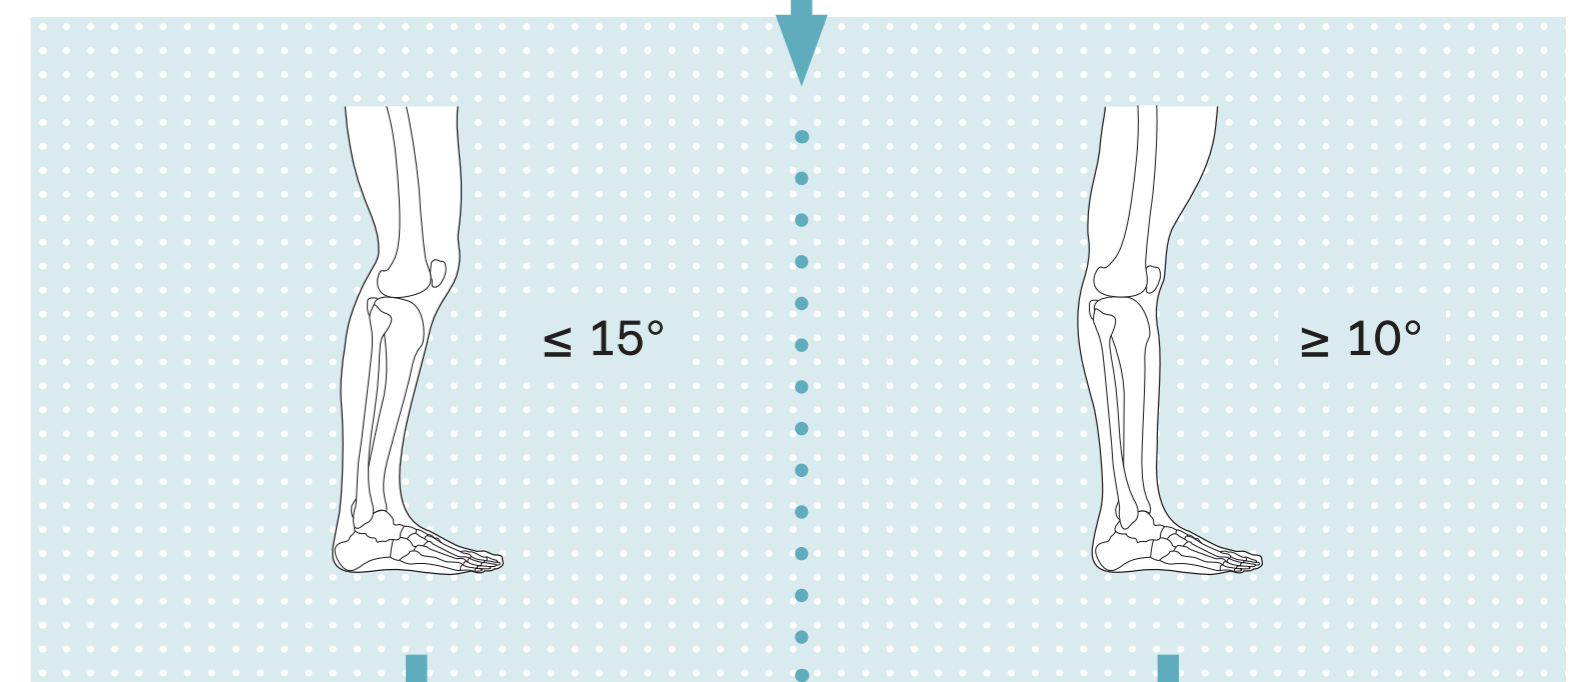
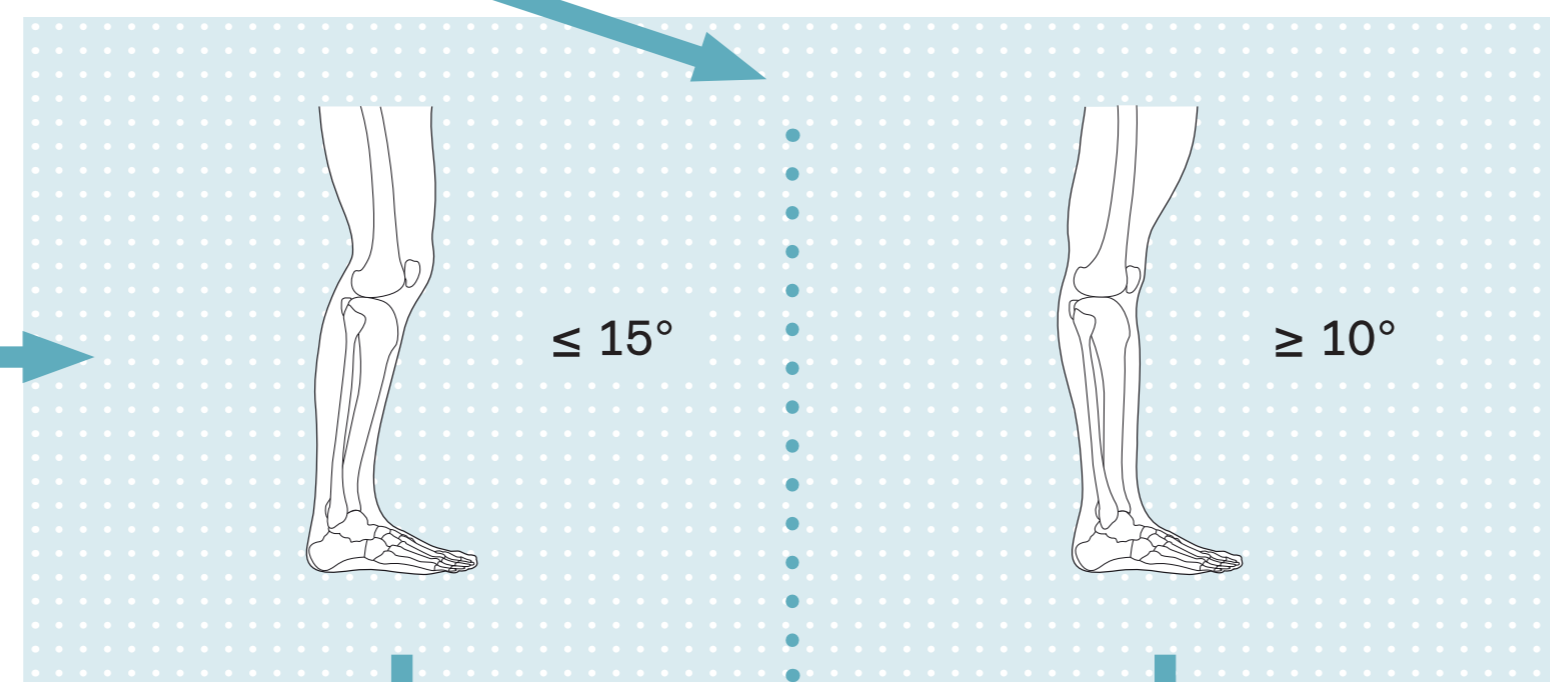
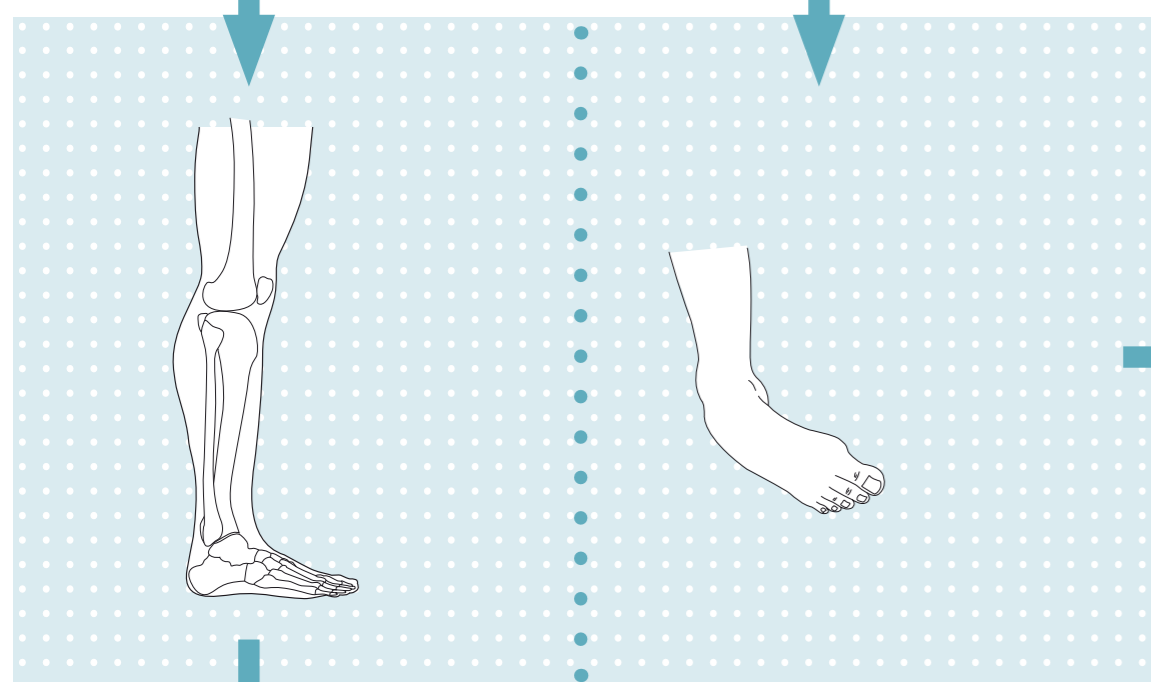


SCO Selection Guide

Stance control orthosis

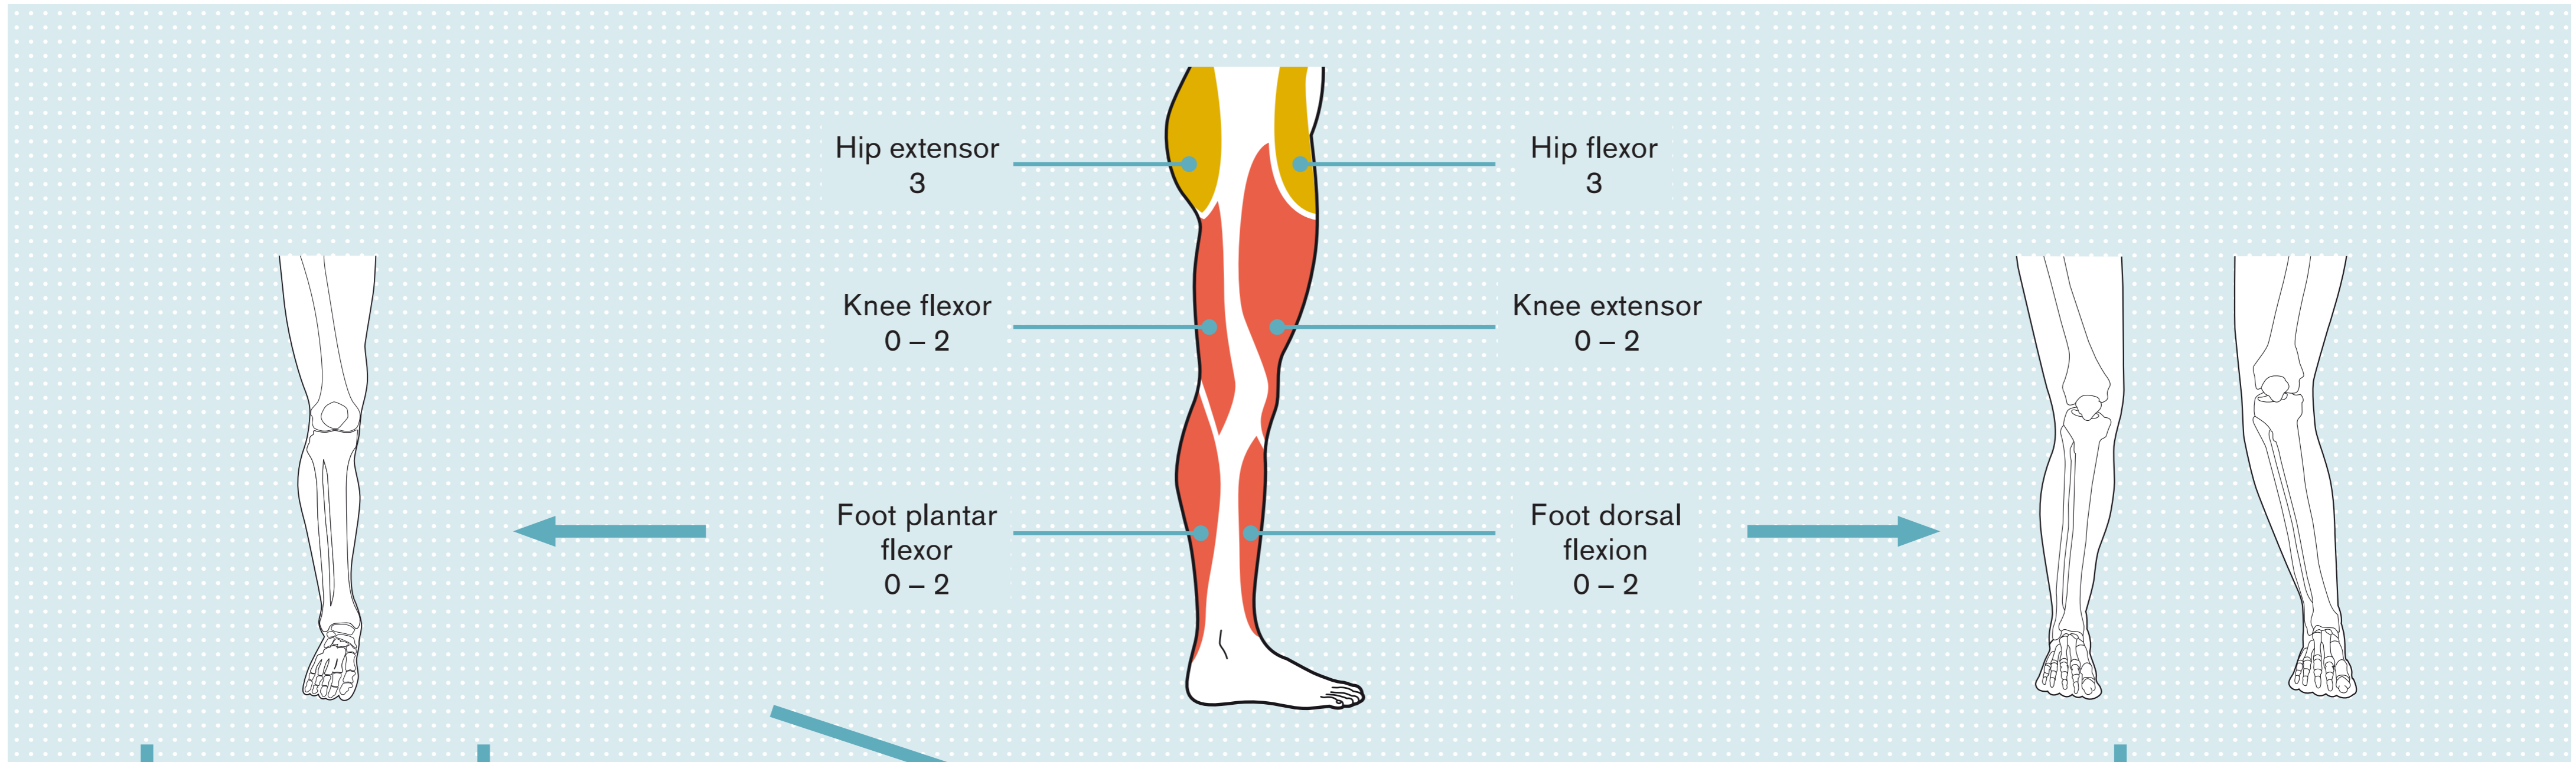




170K1=80* FreeWalk
≤ 176 lbs

170K1=120* FreeWalk
≤ 265 lbs

17B203=* E-MAG Active
≤ 187 lbs

17B206=* Medial support for E-Mag Active

17B203=* E-MAG Active
≤ 220 lbs

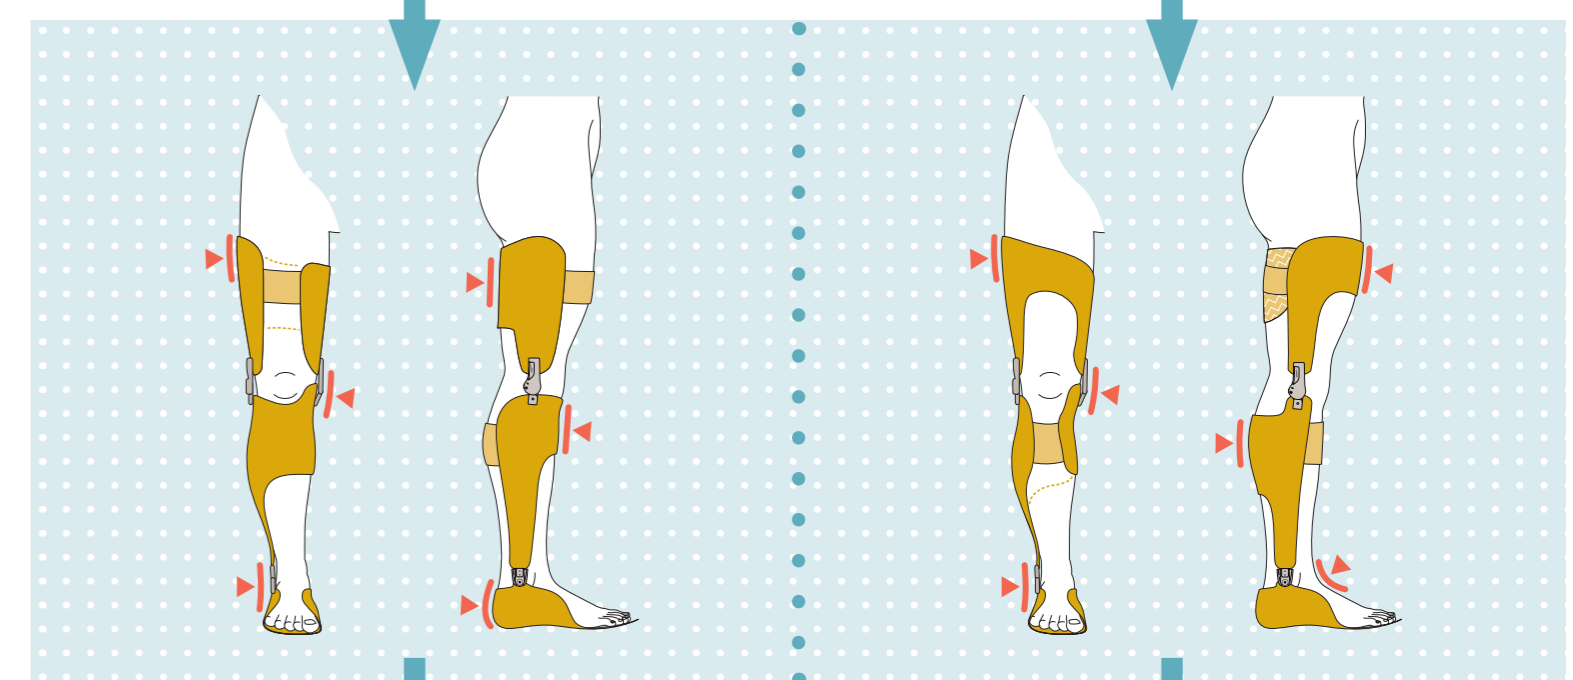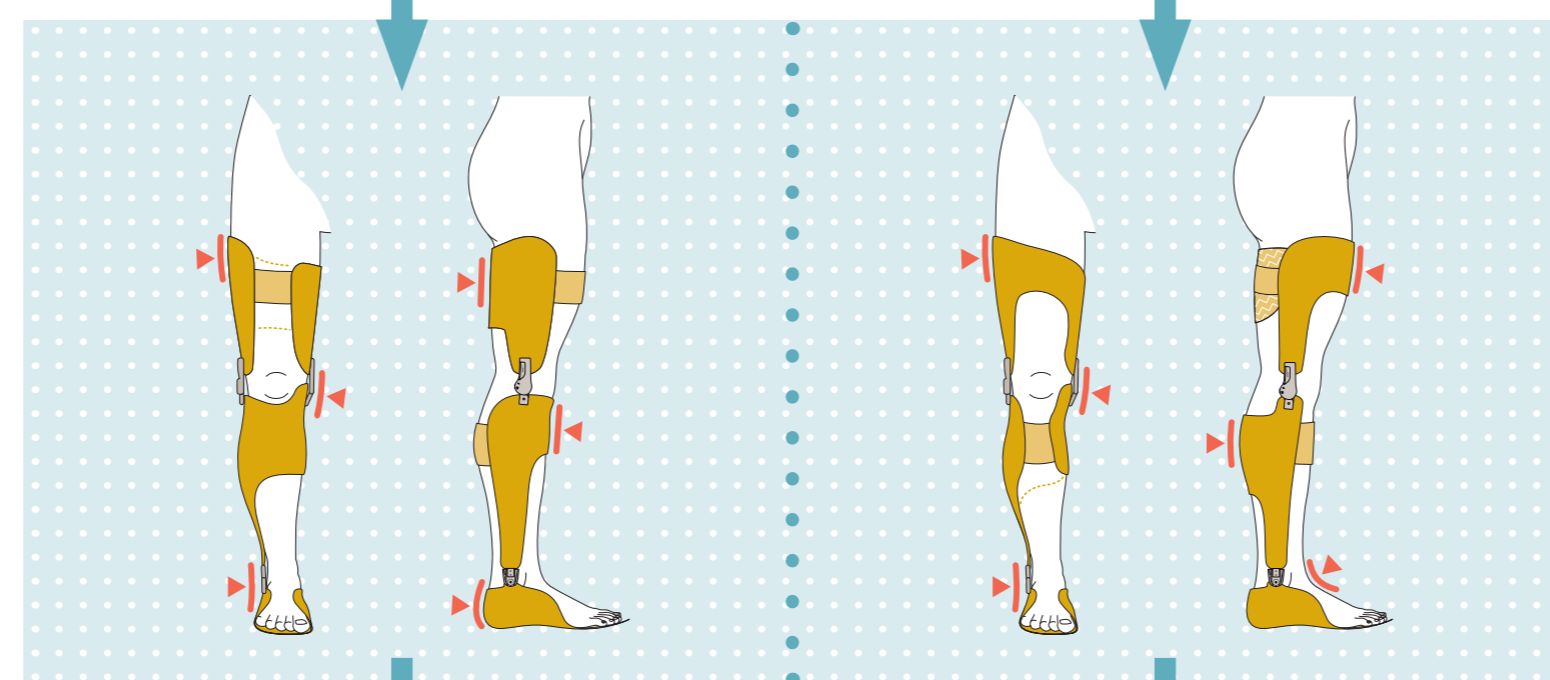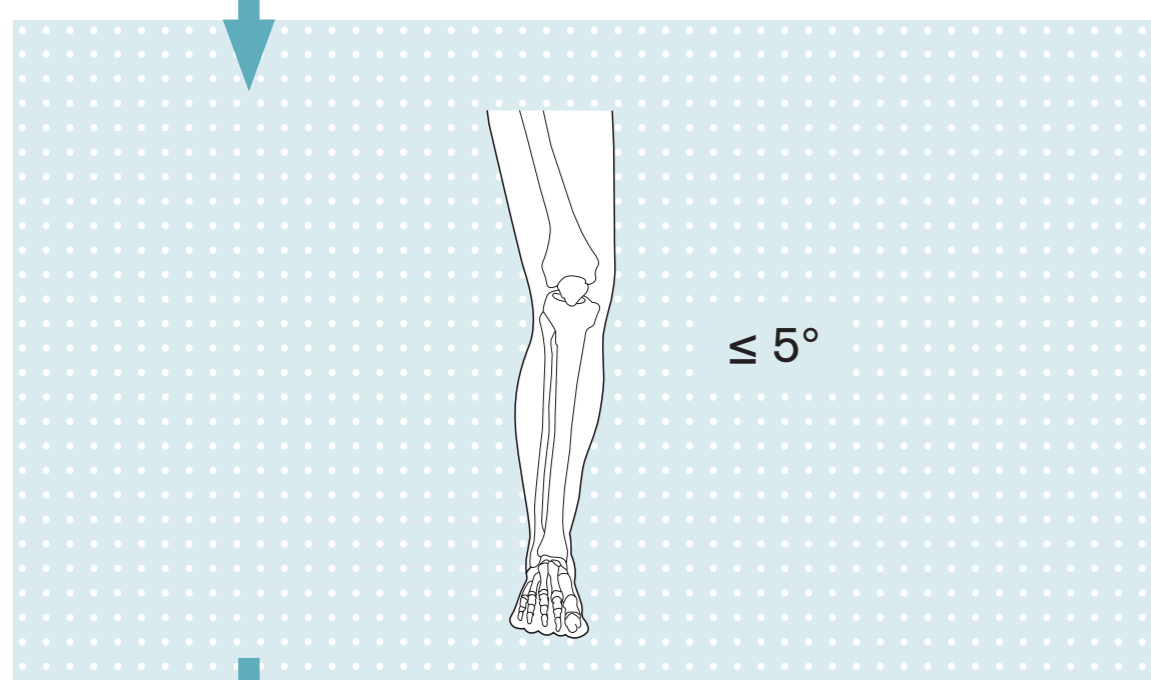

170D30 Medial support for FreeWalk

17LA3N=* Unilateral ankle joint

17LA3N=* Unilateral ankle joint

OR

Energy returning ankle joints
Nexgear Tango and Carbon Ankle Seven

OR

17AD100=* Nexgear Tango
with Reaction Modules and Reaction Springs

17CF1=* Carbon Ankle Seven

17AD100=* Nexgear Tango
with Reaction Modules and Reaction Springs

17CF1=* Carbon Ankle Seven